

LSBio™ Mouse/Human/Rat Phospho-MAPK3 / ERK1 ELISA Kit

Catalog No. LS-F544

User Manual (Revised May 18, 2012)

**Please Read the Manual Carefully
Before Starting your Experiment**



For research use only. Not approved for use in humans or for clinical diagnosis.



**Phospho-Erk1(T202/Y204)/Erk2(T185/Y187)
ELISA Kit Protocol**

TABLE OF CONTENTS

I. Introduction.....	2	II.	
Material Provided.....	3		
III.Storage.....	3		
IV.Additional Materials Required.....	4	V.	
Sample Preparation.....	4		
VI.Reagent Preparation.....	5		
VII.Assay Procedure.....	7		
VIII.Assay Procedure Summary.....	8		
IX.Typical Data.....	9		
i. Positive Control.....	9		
ii. Recombinant human EGF Stimulation of A431 Cell Lines.....	10		
References.....	11	X.	
XI.Troubleshooting Guide.....	12		

I. INTRODUCTION

The Phospho-Erk1(T202/Y204)/Erk2(T185/Y187) ELISA (Enzyme-Linked Immunosorbent Assay) kit is a very rapid, convenient and sensitive assay kit that can monitor the activation or function of important biological pathways in human and mouse cell lysates. By determining phosphorylated Erk1/2 protein in your experimental model system, you can verify pathway activation in your cell lysates. You can simultaneously measure numerous different cell lysates without spending excess time and effort in performing a Western Blotting analysis.

This Sandwich ELISA kit is an in vitro enzyme-linked immunosorbent assay for the measurement of human, mouse and rat phospho-Erk1 (T202/Y204)/Erk2(T185/Y187). An anti-pan Erk1/2 antibody has been coated onto a 96-well plate. Samples are pipetted into the wells and Erk1/2 present in a sample is bound to the wells by the immobilized antibody. The wells are washed and anti-Erk1(T202/Y204)/Erk2(T185/Y187) antibody is used to detect phosphorylated Erk1(T202/Y204)/Erk2(T185/Y187). After washing away unbound antibody, HRP-conjugated anti-rabbit IgG is pipetted to the wells. The wells are again washed, a TMB substrate solution is added to the wells and color develops in proportion to the amount of Erk1(T202/Y204)/Erk2(T185/Y187) bound. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm.

II. MATERIAL PROVIDED

1. Erk1/2 Microplate (Item A): 96 wells (12 strips x 8 wells) coated with anti-pan Erk1/2 antibody.
2. Wash Buffer Concentrate (20x) (Item B): 25 ml of 20x concentrated solution
3. Assay Diluent (Item E): 15 ml of 5x concentrated buffer. For diluting cell lysate sample, detection antibody (Item C-1) and HRP-conjugated anti-rabbit IgG Concentrate (Item D-1).
4. Detection Antibody Erk1(T202/Y204)/Erk2(T185/Y187) (Item C-1): 2 vial of rabbit anti-Erk1(T202/Y204)/Erk2(T185/Y187) (each vial is enough to assay half microplate).
5. HRP-conjugated Anti-rabbit IgG (Item D-1), 25 μ l of 500x concentrated HRP-conjugated anti-rabbit IgG.
6. TMB One-Step Substrate Reagent (Item H): 12 ml of 3,3',5,5'-tetramethylbenzidine (TMB) in buffered solution.
7. Stop Solution (Item I): 8 ml of 0.2 M sulfuric acid.
8. Cell Lysate Buffer (Item J): 5 ml 2x cell lysis buffer (not including protease and phosphatase inhibitors).
9. Positive Control A431S002-1 (Item K): 1 vial of lyophilized powder from A431 cell lysate.

III. STORAGE

Upon receipt, the kit should be stored at -20°C . Please use within 6 months from the date of shipment. After initial use, Wash Buffer Concentrate (Item B), Assay Diluent (Item E), TMB One-

Step Substrate Reagent (Item H), Stop Solution (Item I) and Cell Lysate Buffer (Item J) should be stored at 4°C to avoid repeated freeze-thaw cycles. Return unused wells to the pouch containing desiccant pack, reseal along entire edge and store at -20°C. Item D-1 store at 2-8 °C for up to one month (store at -20 °C for up to 6 months, avoid repeated freeze-thaw cycles). Reconstituted Positive Control (Item K) should be stored at -70°C.

IV. ADDITIONAL MATERIALS REQUIRED

- 1 Microplate reader capable of measuring absorbance at 450 nm.
- 2 Protease and Phosphatase inhibitors.
- 3 Shaker.
- 4 Precision pipettes to deliver 2 µl to 1 ml volumes.
- 5 Adjustable 1-25 ml pipettes for reagent preparation.
- 6 100 ml and 1 liter graduated cylinders.
- 7 Distilled or deionized water.
- 8 Tubes to prepare sample dilutions.

V. SAMPLE PREPARATION

Cell lysates - Rinse cells with PBS, making sure to remove any remaining PBS before adding the Cell Lysate Buffer. Solubilize cells at 4×10^7 cells/ml in 1x Cell Lysate Buffer (we recommend adding protease and phosphatase inhibitors to Cell Lysate Buffer prior to sample preparation). Pipette up and down to resuspend and incubate the lysates with shaking at 2 - 8° C for 30 minutes.

Microcentrifuge at 13,000 rpm for 10 minutes at 2 - 8° C, and transfer the supernates into a clean test tube. Lysates should be used

immediately or aliquoted and stored at $-70\text{ }^{\circ}\text{C}$. Avoid repeated freeze-thaw cycles. Thawed lysates should be kept on ice prior to use.

For the initial experiment, we recommend to do a serial dilution testing such as 5-fold and 50-fold dilution for your cell lysates with 1x Assay Diluent (Item E) before use.

Note: The fold dilution of sample used depends on the abundance of phosphorylated proteins and should be determined empirically. More of the sample can be used if signals are too weak. If signals are too strong, the sample can be diluted further.


Cell Lysate Buffer should be diluted 2-fold with deionized or distilled water before use (recommend to add protease and phosphatase inhibitors).

VI. REAGENT PREPARATION

1. Bring all reagents and samples to room temperature ($18 - 25^{\circ}\text{C}$) before use.
2. Item D, Assay Diluent should be diluted 5-fold with deionized or distilled water before use.
3. Preparation of Positive Control: Briefly spin the Positive Control vial of Item K. Add $600\text{ }\mu\text{l}$ 1x Assay Diluent (Item E, Assay Diluent should be diluted 5-fold with deionized or distilled water before use) into Item K vial to prepare Positive Control (P-1) solution. **Dissolve the powder thoroughly by a gentle**

mix (it can be removed by centrifuge if any precipitate in the solution is found). Pipette 400 μ l 1x Assay Diluent into each tube. Use the Positive Control (P-1) solution to produce a dilution series (shown below). Mix each tube thoroughly before the next transfer. 1x Assay Diluent serves as the background. (See i. Positive Control of part IX. TYPICAL DATA for a typical result in page 9).

Positive Control, Item K +
600 μ l 1x Assay Diluent

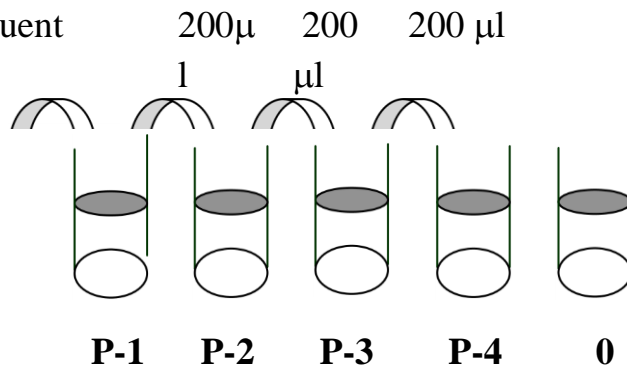

4. If the Wash Concentrate (20x) (Item B) contains visible crystals, warm to room temperature and mix gently until dissolved. Dilute 20 ml of Wash Buffer Concentrate into deionized or distilled water to yield 400 ml of 1x Wash Buffer.
5. Briefly spin the detection antibody (Item C-1) before use. Add
Add 100 μ l of 1x Assay Diluent into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can be stored at 4°C for 5 days or at –80°C for one month). The rabbit anti-Erk1(T202/Y204)/Erk2(T185/Y187) antibody should be diluted 55-fold with 1x Assay Diuent and used in step 4 of Part VII Assay Procedure.

6. Briefly spin the HRP-conjugated anti-rabbit IgG (Item D-1) before use. Pipette up and down to mix gently. HRP-conjugated anti-rabbit IgG concentrate should be diluted 500-fold with 1x Assay Diluent.

For example: Briefly spin the vial (Item D-1) and pipette up and down to mix gently. Add 10 μ l of HRP-conjugated anti-rabbit IgG concentrate into a tube with 5.0 ml 1x Assay Diluent to prepare a 500-fold diluted HRP-conjugated anti-rabbit IgG solution.

7. Cell Lysate Buffer should be diluted 2-folds with deionized or distilled water before use (recommend to add protease and phosphatase inhibitors).

VII. ASSAY PROCEDURE:

1. Bring all reagents to room temperature (18 - 25°C) before use. It is recommended that all samples or Positive Control should be run at least in duplicate.
2. Add 100 μ l of each sample or positive control into appropriate wells. Cover well with plate holder and incubate for 2.5 hours at room temperature or over night at 4°C with shaking.
3. Discard the solution and wash 4 times with 1x Wash Solution. Wash by filling each well with Wash Buffer (300 μ l) using a multi-channel pipette or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or

decanting. Invert the plate and blot it against clean paper towels.

4. Add 100 μ l of prepared 1x detection antibody anti-Erk1(T202/Y204)/Erk2(T185/Y187) (Reagent Preparation step 5) to each well. Incubate for 1 hour at room temperature with shaking.
5. Discard the solution. Repeat the wash as in step 3.
6. Add 100 μ l of prepared 1x HRP-conjugated anti-rabbit IgG (see Reagent Preparation step 6) to each well. Incubate for 1 hour at room temperature with shaking.
7. Discard the solution. Repeat the wash as in step 3.
8. Add 100 μ l of TMB One-Step Substrate Reagent (Item H) to each well. Incubate for 30 minutes at room temperature in the dark with shaking.
9. Add 50 μ l of Stop Solution (Item I) to each well. Read at 450 nm immediately.

VIII. ASSAY PROCEDURE SUMMARY

1. Prepare all reagents, samples and standards as instructed.



2. Add 100 μ l sample or positive control to each well.

Incubate 2.5 hours at room temperature or over night at 4°C.



3. Add 100 μ l prepared primary antibody to each well.
Incubate 1.0 hours at room temperature.



4. Add 100 μ l prepared 1X HRP-Streptavidin solution.
Incubate 1 hour at room temperature.



5. Add 100 μ l TMB One-Step Substrate Reagent to each well.
Incubate 30 minutes at room temperature.



6. Add 50 μ l Stop Solution to each well.
Read at 450 nm immediately.

IX. TYPICAL DATA

ELISA data analysis: Average the duplicate readings for each sample or positive.

i. Positive Control

A431 cells were treated with recombinant human EGF at 37°C for 20 min. Solubilize cells at 4×10^7 cells/ml in Cell Lysate Buffer. Serial dilutions of lysates were analyzed in this ELISA. Please see step 3 of Part VI Reagent Preparation for detail.


Assay Diluent

10

OD=450 nm

--	--	--	--	--	--

B). Western-Blot Analysis

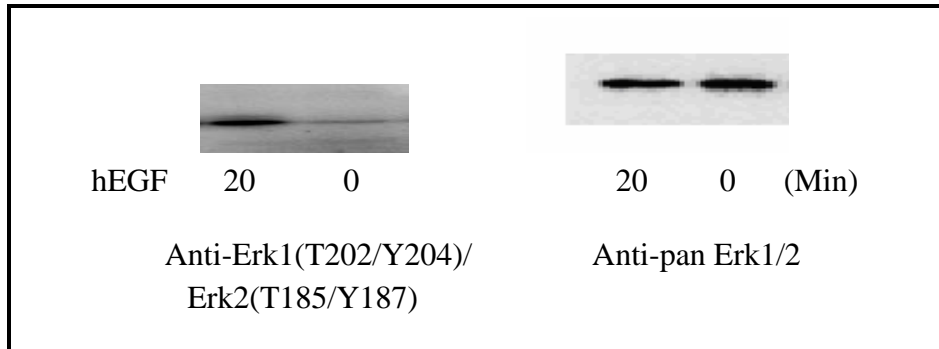

X. REFERENCES:

1. Boulton TG, Cobb MH. Identification of multiple extracellular signal-regulated kinases (ERKs) with antipeptide antibodies. *Cell Regul.* 1991; 2(5):357-371.
2. Meng J, Casey PJ. Activation of Gz attenuates Rap1-mediated differentiation of PC12 cells. *J Biol Chem.* 2002; 277(45):43417-43424.
3. Ackerley S, Grierson AJ, Brownlee J, et al. Glutamate slows axonal transport of neurofilaments in transfected neurons. *J Cell Biol.* 2000; 150(1):165-175.

XI. TROUBLESHOOTING GUIDE

Problem	Cause	Solution
1. Sample signals: a. Too low b. Too high	a. Sample concentration is too low b. Sample concentration is too high	a. Increasing sample concentration b. Reducing sample concentration
2. Large CV	a. Inaccurate pipetting	a. Check pipettes
3. High background	a. Plate is insufficiently washed b. Contaminated wash buffer	a. Review the manual for proper washing. If using an automated plate washer, check that all ports are unobstructed. b. Make fresh wash buffer
4. Positive Control: Low signal	a. Improper storage of the ELISA kit b. Stop solution c. Improper primary or secondary antibody dilution	a. Upon receipt, the kit should be stored at -20°C . Store the positive control at -70°C after reconstitution. b. Stop solution should be added to each well before measurement and read OD immediately. c. Ensure correct dilution

Important Note: During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. We recommend briefly centrifuging the vial to dislodge any liquid in the container's cap prior to opening.

Warning: This reagent may contain sodium azide and sulfuric acid. The chemical, physical, and toxicological properties of these materials have not been thoroughly investigated. Standard Laboratory Practices should be followed. Avoid skin and eye contact, inhalation, and ingestion. Sodium azide forms hydrazoic acid under acidic conditions and may react with lead or copper plumbing to form highly explosive metal azides. On disposal, flush with large volumes of water to prevent accumulation.

Returns, Refunds, Cancellations: Any problems with LifeSpan products must be reported to LifeSpan within 10 days of product receipt. The customer must obtain written authorization from LifeSpan before returning items. To request that goods be returned, please contact LifeSpan Technical Support. If an error by LifeSpan BioSciences results in shipment of an incorrect order, LifeSpan will, at its option, either ship a replacement order at no charge, or credit the customer's account for the original product shipped in error. Returns and cancellations may be subject to a 30% restocking fee.

Conditions & Warranty: All LifeSpan products are intended for Research Use Only and are not for use in human therapeutic or diagnostic applications. The information supplied with each product is believed to be accurate, but no warranty or guarantee is offered for the products, because the ultimate conditions of use are beyond LifeSpan's control. The information supplied with each product is not to be construed as a recommendation to use this product in violation of any patent, and LifeSpan will not be held responsible for any infringement or other violation that may occur with the use of its products. Under no event will LifeSpan be responsible for any loss of profit or indirect consequential damage, including, but not limited to, personal injuries resulting from use of these products. LifeSpan's liability to any user of Products for damages that do not result from any fault of the user, will be limited to replacement of the Product(s) only, and in no event shall LifeSpan's liability exceed the actual price received by LifeSpan for the Product(s) at issue. LifeSpan shall not be liable for any indirect, special, incidental or consequential damages. LIFESPAN FURTHER DISCLAIMS ANY AND ALL EXPRESS AND IMPLIED OR STATUTORY WARRANTIES WITH RESPECT TO THE PRODUCTS, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE. LifeSpan disclaims any and all responsibility for any injury or damage which may be caused by the fault of the user.

For research use only. Not approved for use in humans or for clinical diagnosis.



2401 Fourth Avenue Suite 900 Seattle, WA 98121

Tel: 206.374.1102

Fax: 206.577.4565

Technical.Support@LSBio.com