

LSBio™ Human Phospho-EGFR Cell-Based ELISA Kit

Catalog No. LS-F940

User Manual

**Please Read the Manual Carefully
Before Starting your Experiment**



For research use only. Not approved for use in humans or for clinical diagnosis.

Cell-Based Human EGFR (Tyr1068)
Phosphorylation ELISA Kit

TABLE OF CONTENTS

I. Introduction.....	2
II. How It Works.....	3
III. Reagents and Storage.....	4
IV. Additional Reagents Required.....	4
V. Reagent Preparation	5
VI. Assay Procedure	6 VII.
Assay Procedure Summary	9 VIII.
Quality Control Data	10 IX.
References	12 X.
Troubleshooting Guide	13

I. INTRODUCTION

Protein phosphorylation is instrumental in the regulation of protein activity within a cell. It plays important roles in the living cells including proliferation, differentiation and metabolism. A large number of protein kinases and phosphatases have been extensively investigated, and have been shown to be involved in signal transduction pathways.

The LSBio® Cell-Based Human EGFR (Tyr1068) Phosphorylation ELISA kit is a very rapid, convenient and sensitive assay kit that can monitor the activation or function of important biological pathways in cells. It can be used for measuring the relative amount of EGFR (Tyr1068) phosphorylation and screening the effects of various treatments, inhibitors (such as siRNA or chemicals), or activators in cultured human cell lines. By determining EGFR protein phosphorylation in your experimental model system, you can verify pathway activation in your cell lines without spending excess time and effort in preparing cell lysate and performing an analysis of Western Blot. In the Cell-Based EGFR (Tyr1068) ELISA kit, cells are seeded into a 96 well tissue culture plate. The cells are fixed after various treatments, inhibitors or activators. After blocking, Anti-Phospho-EGFR (Tyr1068) or Anti-EGFR (primary antibody) is pipetted into the wells and incubated. The wells are washed, and HRP-conjugated anti-rabbit IgG (secondary antibody) is added to the wells. The wells are washed again, a TMB substrate solution is added to the wells and color develops in proportion to the amount of protein. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm.

See Figure 1 below for an illustration.

II. HOW IT WORKS

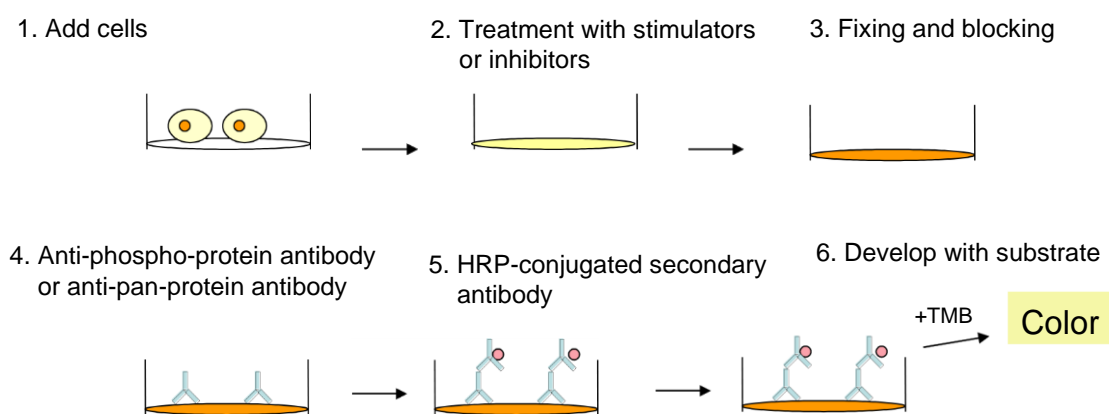


Fig.1. Cell-Based protein phosphorylation procedure

III. REAGENTS AND STORAGE

Store entire kit at $\leq -20\text{ }^{\circ}\text{C}$ immediately upon arrival. Kit must be used within the 6 month expiration date. Avoid repeated freeze-thaw cycles.

ITEM	COMPONENT	1 PLATE KIT	2 PLATE KIT	STORAGE AFTER INITIAL THAW*
A	Uncoated 96-Well Microplate	1 plate	2 plates	Room Temperature
B	20X Wash Buffer A Concentrate	1 vial (30 ml)		2-8 °C
C	20X Wash Buffer B Concentrate	1 vial (30 ml)		
D	Fixing Solution	1 vial (30 ml)		
E	30X Quenching Buffer Concentrate	1 vial (2 ml)		
F	5X Blocking Buffer Concentrate	1 vial (20 ml)		
G	1000X Rabbit Anti-phospho (Tyr1068) EGFR Concentrate	1 vial (6 μl)	2 vials (6 μl /ea)	-20 °C
H	1000X Rabbit Anti-EGFR Concentrate	1 vial (6 μl)	2 vials (6 μl /ea)	
I	2000X HRP Conjugated Anti-Rabbit IgG Concentrate	1 vial (10 μl)	2 vials (10 μl /ea)	
J	TMB Substrate	1 vial (12 ml)	2 vials (12 ml/ea)	2-8 °C
K	Stop Solution**	1 vial (14 ml)		

*For up to 3 months (unless otherwise stated) or until expiration date.

**Contains 0.2 M Sulfuric Acid

IV. ADDITIONAL MATERIALS REQUIRED

1. A model cell line, protein tyrosine kinase inhibitors, growth factors or cytokines
2. Microplate reader capable of measuring absorbance at 450 nm
3. 37 °C incubator
4. Precision pipettes to deliver 2 μl to 1 ml volumes
5. Adjustable 1-25 ml pipettes for reagent preparation
6. 100 ml and 1 liter graduated cylinders
7. Absorbent paper
8. Distilled or deionized water
9. Orbital shaker or oscillating rocker

V. REAGENT PREPARATION

NOTE: Thaw all reagents to room temperature immediately before use. If wash buffers contain visible crystals, warm to room temperature and mix gently until dissolved.

NOTE: Briefly centrifuge (~1,000g) ITEMS G, H, and I before opening to ensure maximum recovery.

	ITEM	COMPONENT	PREPARATION	EXAMPLE
	A	Uncoated 96-Well Microplate	No Preparation	N/A
	B	20X Wash Buffer A Concentrate	Dilute each 20-fold with distilled or deionized water	25 ml of concentrate + 475 ml of water = 500 ml of 1X working solution
	C	20X Wash Buffer B Concentrate		
	D	Fixing Solution	No Preparation	N/A
	E	30X Quenching Buffer Concentrate	Dilute 30-fold with 1X Wash Buffer A	1 ml of concentrate + 29 ml of wash buffer = 30 ml of 1X working solution
	F	5X Blocking Buffer Concentrate	Dilute 5-fold with distilled or deionized water	20 ml of concentrate + 80 ml of water = 100 ml of 1X working solution
PRIMARY ANTIBODY	G	1000X Rabbit Anti-phospho (Tyr1068) EGFR Concentrate	Dilute each 1000-fold with 1X Blocking Buffer	6 μ l of concentrate + 5594 μ l of 1X Blocking Buffer = 6 ml of 1X working solution
	H	1000X Rabbit Anti-EGFR Concentrate		
SECONDARY ANTIBODY	I	2000X HRP Conjugated Anti-Rabbit IgG Concentrate	Dilute 2000-fold with 1X Blocking Buffer	10 μ l of concentrate + 19990 μ l of 1X Blocking Buffer = 20 ml of 1X working solution
	J	TMB Substrate	No Preparation	N/A
	K	Stop Solution		

VI. ASSAY PROCEDURE:

NOTE: *ALL incubations and wash steps must be performed under gentle rocking or rotation (~1-2 cycles/sec).*

1. Design your experiment. For example, see Figure 2 below.

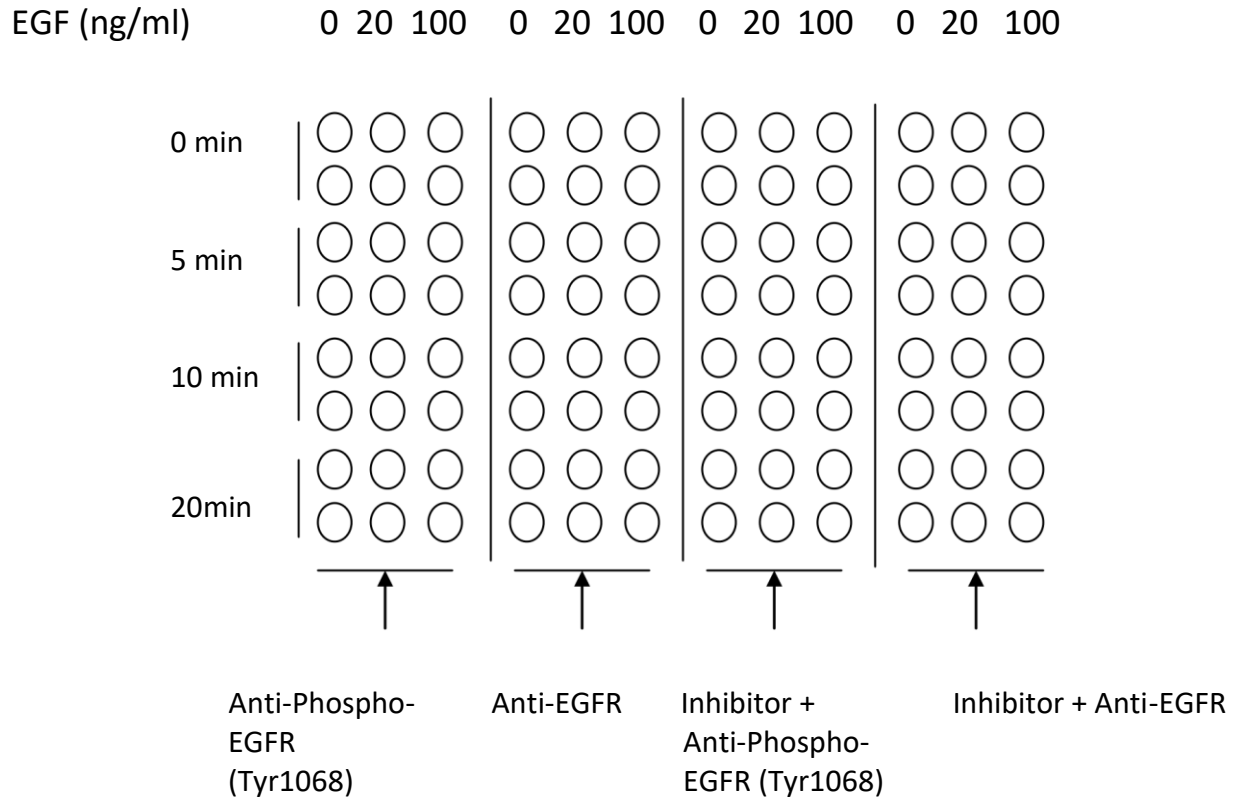


Fig. 2. Example of how to seed cells for LSBio® cell-based assay

OPTIONAL: *If seeding HUVECs, HMEC-1 or other loosely attached cells, coat the Uncoated 96-Well Microplate (ITEM A) by adding 100 µl poly-L-Lysine (Recommended Sigma Aldrich, Cat#: P4832) into each well and then follow manufacturer's instructions. A pre-coated CellBIND® microplate or other poly-lysine treated tissue culture plate may be used in place of Item A.*

2. Seed 100 μ l of 20,000 cells into each well of the Uncoated 96-Well Microplate (ITEM A) provided and incubate overnight at 37°C with 5% CO₂.

NOTE: *The optimal cell number used will vary on the cell line and the relative amount of protein phosphorylation. More or less cells may be used but this must be determined empirically.*

NOTE: *The cells can be starved ~4-24 hours (depending on cell line) prior to treatment with inhibitors or activators.*

3. Apply various treatments, inhibitors (such as siRNA or chemicals) or activators according to manufacturer's instructions and incubate for the desired time points.

NOTE: *It is recommended to dissolve inhibitors or activators into serum-free cell culture medium before treating the cells (unless otherwise stated in the manufacturer's instructions.)*

4. Discard the cell culture medium by flipping the microplate upside down and **gently** tapping the bottom of the microplate over a sink.

5. Wash by pipetting 200 μ l of the **prepared 1X** Wash Buffer A (see Section V. Reagent Preparation) into each well. Discard the wash buffer (same as step 4) and wash 2 more times for a total of 3 washes using fresh wash buffer each time. After the final wash, gently blot the microplate onto a paper towel to remove any excess/remaining buffer.

NOTE: *To avoid cell loss, do not pipette directly onto the cells. Instead, gently dispense the liquid down the wall of cell culture wells. Also avoid the use of vacuum suction or too forcefully tapping the microplate when discarding any solution.*

6. Add 100 μ l of Fixing Solution (ITEM D) into each well and incubate for 20 minutes at room temperature.

NOTE: *The fixing solution is used to permeabilize the cells.*

7. Repeat wash step 5.

8. Add 200 μ l of the **prepared1X** Quenching Buffer (ITEM E) into each well and incubate 20 minutes at room temperature.

NOTE: *The quenching buffer is used to minimize the background response.*

9. Wash **4** times with 1X Wash Buffer A.

10. Add 200 μ l of the **prepared1X** Blocking Buffer (see Section V. Reagent Preparation) into each well and incubate for 1 hour at 37°C.

11. Wash **3** times with the **prepared1X** Wash Buffer B (ITEM C).

NOTE: *If needed, the microplate may be stored at -80°C for several days after this wash.*

12. Add 50 μ l of the **prepared1X** primary antibody (ITEM G or H) into each corresponding well and incubate for 2 hours at room temperature.

13. Repeat step 11.

14. Add 50 μ l of **1X** HRP Conjugated secondary antibody (ITEM I) into each well and incubate for 1 hour at room temperature.

15. Wash **3** times with 1X Wash Buffer B.

16. Add 100 μ l of the TMB Substrate (ITEM J) into each well and incubate for 30 minutes at room temperature **in the dark**.

17. Add 50 μ l of the Stop Solution (ITEM K) into each well. Read at 450 nm immediately.

VII. ASSAY PROCEDURE SUMMARY

1. Seed 20,000 cells into each well and incubate overnight.



2. Apply various treatment, inhibitors or activators according to manufacturer's instructions.



3. Add 100 μ l of Fixing Solution into each well and incubate for 20 minutes at room temperature.



4. Add 200 μ l of prepared 1X Quenching Buffer and incubate for 20 minutes at room temperature.



5. Add 200 μ l of prepared 1X Blocking Buffer and incubate for 1 hour at 37°C.



6. Add 50 μ l of prepared 1X primary antibody to each well and incubate for 2 hours at room temperature.



7. Add 50 μ l of prepared 1X HRP Conjugated secondary antibody and incubate for 1 hour at room temperature.



8. Add 100 μ l TMB Substrate and incubate 30 minutes at room temperature.



9. Add 50 μ l Stop Solution to each well. Read at 450 nm immediately.

VIII. QUALITY CONTROL DATA

Representative results of Cell-Based EGFR (Tyr1068) are shown below:

1. Seeded 20,000 A431 cells into appropriate wells of the microplate. Cells were incubated at 37°C in 5% CO₂ overnight.
2. Added 50 μ l of different concentrations of stimulators (rhEGF concentration for A431 cells: 0, 20 or 100 ng/ml in serum free DMEM) to appropriate wells (shown below). Then incubated for 10 min at 37°C.
3. Discarded the solution and wash 3 times with 1X Wash Buffer A (200 μ l each) immediately. Then tapped the plate upside down to remove all of excess wash buffer. The protocol was then followed as stated.

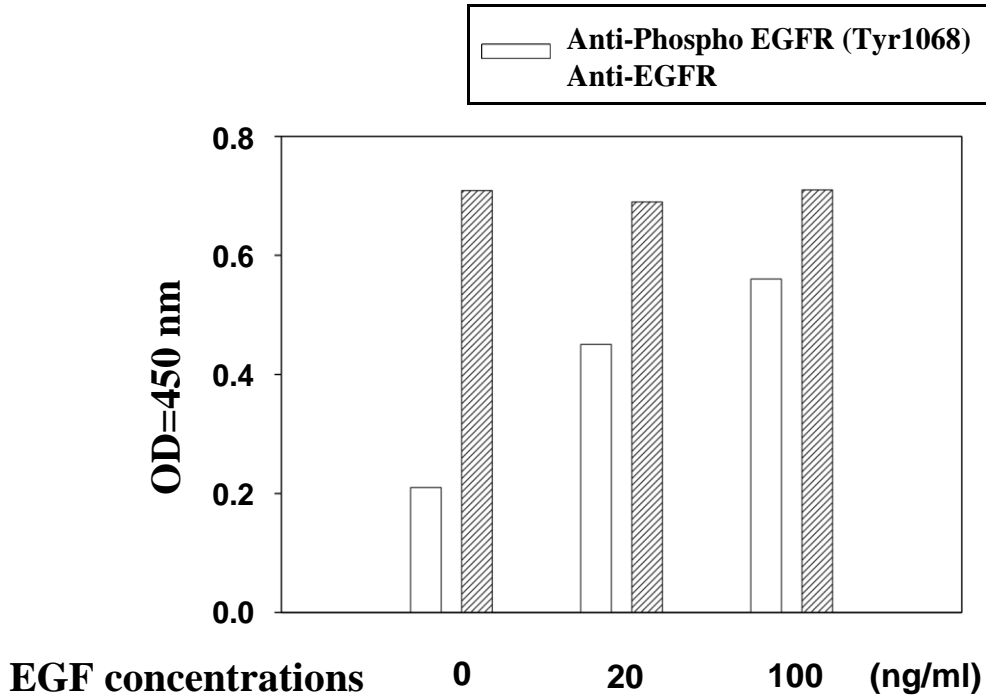


Fig. 3. A431 cells were stimulated by different concentrations of EGF for 10 min at 37oC

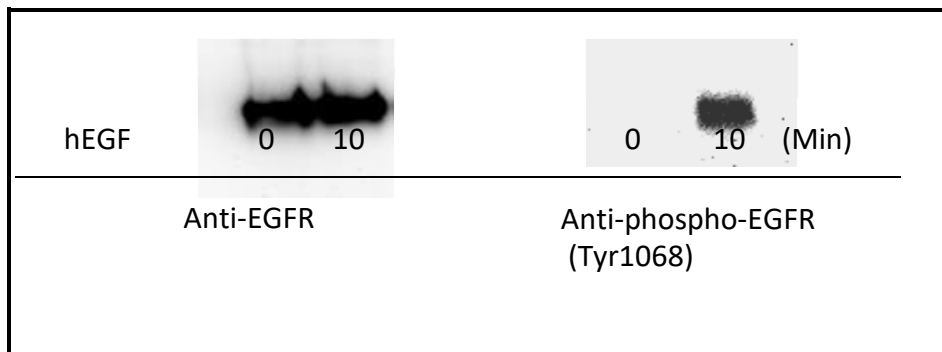


Fig. 4. Western blot analysis of extracts from 100 ng/ml hEGF treated A431 cells. Phospho-EGFR (Tyr1068) and EGFR antibodies were used in both detection assays.

IX. REFERENCES:

1. Hubbard, S.R. et al. (1994) *Nature* 372, 746–754.
2. Hackel, P.O. et al. (1999) *Curr. Opin. Cell Biol.* 11, 184–189.
3. Levkowitz, G. et al. (1999) *Mol. Cell* 4, 1029–1040.
4. Zwick, E. et al. (1999) *Trends Pharmacol. Sci.* 20, 408–412.
5. Biscardi, J.S. et al. (1999) *J. Biol. Chem.* 274, 8335–8343.

X: TROUBLESHOOTING GUIDE

Problem	Cause	Solution
1. Low signal	1. Improper storage of the ELISA kit	1. Store the kit according to manual instructions. Keep substrate solution in dark.
	2. Improper dilution	2. Ensure correct preparation of antibody and reagents.
	3. Cells drop off from the wells	3. Some of treatments may make cells drop off the wells. Reduce inhibitor or activator concentration.
2. High background	1. Inadequate washing	1. Be sure to remove all of washing solution and follow the recommendation for washing.
	2. Too much cells	2. Reduce the cell number
3. Large CV	1. Inaccurate pipetting	1. Check pipette.
	2. Remaining wash buffer in the well	2. Remove all of wash buffer.
	3. Cells drop off from the wells	3. Please don't directly face the cells with tips when adding reagents or wash buffer.

Important Note: During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. We recommend briefly centrifuging the vial to dislodge any liquid in the container's cap prior to opening.

Warning: This reagent may contain sodium azide and sulfuric acid. The chemical, physical, and toxicological properties of these materials have not been thoroughly investigated. Standard Laboratory Practices should be followed. Avoid skin and eye contact, inhalation, and ingestion. Sodium azide forms hydrazoic acid under acidic conditions and may react with lead or copper plumbing to form highly explosive metal azides. On disposal, flush with large volumes of water to prevent accumulation.

Returns, Refunds, Cancellations: Any problems with LifeSpan products must be reported to LifeSpan within 10 days of product receipt. The customer must obtain written authorization from LifeSpan before returning items. To request that goods be returned, please contact LifeSpan Technical Support. If an error by LifeSpan BioSciences results in shipment of an incorrect order, LifeSpan will, at its option, either ship a replacement order at no charge, or credit the customer's account for the original product shipped in error. Returns and cancellations may be subject to a 30% restocking fee.

Conditions & Warranty: All LifeSpan products are intended for Research Use Only and are not for use in human therapeutic or diagnostic applications. The information supplied with each product is believed to be accurate, but no warranty or guarantee is offered for the products, because the ultimate conditions of use are beyond LifeSpan's control. The information supplied with each product is not to be construed as a recommendation to use this product in violation of any patent, and LifeSpan will not be held responsible for any infringement or other violation that may occur with the use of its products. Under no event will LifeSpan be responsible for any loss of profit or indirect consequential damage, including, but not limited to, personal injuries resulting from use of these products. LifeSpan's liability to any user of Products for damages that do not result from any fault of the user, will be limited to replacement of the Product(s) only, and in no event shall LifeSpan's liability exceed the actual price received by LifeSpan for the Product(s) at issue. LifeSpan shall not be liable for any indirect, special, incidental or consequential damages. LIFESPAN FURTHER DISCLAIMS ANY AND ALL EXPRESS AND IMPLIED OR STATUTORY WARRANTIES WITH RESPECT TO THE PRODUCTS, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE. LifeSpan disclaims any and all responsibility for any injury or damage which may be caused by the fault of the user.

For research use only. Not approved for use in humans or for clinical diagnosis.



2401 Fourth Avenue Suite 900 Seattle, WA 98121

Tel: 206.374.1102

Fax: 206.577.4565

Technical.Support@LSBio.com